



PeliKine Compactä human IL-13 ELISA kit

288 tests

An enzyme immunoassay for the quantitative determination
of human Interleukin 13

PRODUCT INFORMATION

Sanquin Reagents

PO Box 9190
1006 AD Amsterdam
The Netherlands

reagents@sanquin.nl
www.sanquin.nl

Cat.No. **M1913**

For The Netherlands

Tel. 020 - 512 3599
Fax. 020 - 512 3570

For other countries:

Contact your local distributor

I. INTRODUCTION

Interleukin 13 (IL-13) is an immunoregulatory protein produced by activated T-cells. The protein encoded by the IL-13 cDNA is the human homologue of a mouse TH2 product called P600 [1-3]. IL-13 shares many of its biological activities with the TH2 cytokine Interleukin 4; both cytokines are able to enhance expression of CD23 on monocytes and B-cells and also induce IgE production [3-8]. Production of many LPS-induced monokines, such as IL-1 α , IL-1 β , IL-6, IL-8, IL-10, TNF α , IFN α , MIP-1 α , GM-CSF and G-CSF are inhibited by IL-13 [3,6], whereas IL-1ra is upregulated. These properties are shared with IL-4 and IL-10. Therefore IL-4 and IL-13 can be considered as anti-inflammatory molecules. In contrast to IL-4, IL-13 has no growth-promoting effect on T-cells and cannot compete for IL-4 binding to a human T-cell line. Therefore it was thought that the specific receptor for IL-13 is lacking on T-cells [4,9]. However, recently an inhibitory effect of IL-13 on IL-8- and RANTES-induced chemotaxis of T-cells has been described, indicating that T-cells do respond to IL-13 [10], possibly by inhibition of production of the TH1 inducer IL-12 [4].

Bioassays for the quantification of IL-13, including the proliferative assay of an IL-13-dependent subclone of the B9 cell line [12] can be used. However, IL-13 shares many of the biological effects of IL-4 and for this reason the two commonly interfere in bioassays.

Furthermore, these bioassay, although sensitive, are time consuming and susceptible to interference by other substances.

The Pelikine compact™ human IL-13 ELISA kit [11] has been developed for faster, more reproducible and specific quantification of human IL-13 in serum, plasma and other body fluids, as well as in cell-culture supernatant.

II. PRINCIPLE OF THE TEST

The Pelikine compact™ human IL-13 ELISA kit is a "sandwich-type" of enzyme immunoassay in which a monoclonal anti human IL-13 antibody is bound onto polystyrene microtiter wells. Human IL-13, present in a measured volume of sample or standard is captured by the antibody on the microtiter plate, and non-bound material is removed by washing. Subsequently, a biotinylated second monoclonal antibody to human IL-13 is added. This antibody binds to the IL-13 antibody complex present in the microtiter well. Excess biotinylated antibody is removed by washing, followed by addition of horseradish peroxidase (HRP) conjugated streptavidin, which binds onto the biotinylated side of the IL-13 sandwich. After removal of non-bound HRP conjugate by washing, a substrate solution is added to the wells. A coloured product is formed in proportion to the amount of IL-13 present in the sample or standard. After the reaction has been terminated by the addition of a stop solution, absorbance is measured in a microtiter plate reader. From the absorbance of samples and those of a standard curve, the concentration of IL-13 can be determined by interpolation with the standard curve.

III. STORAGE AND STABILITY

The PeliKine compact™ human IL-13 ELISA kit should be stored at -18°C to -32°C. The performance of the kit is guaranteed until the expiration date shown on the case label.

IV. CONTENTS OF THE KIT

The PeliKine compact™ human IL-13 ELISA kit contains material sufficient for 288 tests, including standard curve samples. The reagents provided are:

Quantity	Kit component		Volume	Cap colour
1 vial	coating antibody	100-fold concentrated	375 μ l	red
1 vial	blocking reagent	50-fold concentrated	2 ml	transparent
1 vial	IL-13 standard (lyophilized)	1000 pg/ml	500 μ l	
1 vial	biotinylated antibody	100-fold concentrated	375 μ l	yellow
1 vials	streptavidin-HRP conjugate	10,000-fold concentrated	20 μ l	brown
1 bottle	dilution buffer	5-fold concentrated	60 ml	-
3 pcs	microtiter plates + lid	-	-	-
10 pcs	plate seals	-	-	-

V. PRECAUTIONS FOR USE

- 1) The PeliKine compact™ human IL-13 ELISA kit is intended *for research purposes only*.
- 2) Only use the reagents and microtiter plates supplied with the kit, do not mix reagents from different kit lots.
- 3) Handle all plasma and serum samples with care to prevent transmission of blood-borne infections.
- 4) Sodium azide inactivates HRP, do not use sodium azide-containing solutions, nor add sodium azide to the supplied materials.
- 5) All reagents contain thiomersal (0.001 % w/v) and may be toxic upon ingestion, inhalation or skin contact. Avoid contact of skin, eyes or clothing with dilution, washing or substrate buffer. In case of contact, wash skin or eyes with water and consult a physician.
- 6) Centrifuge all vials before use (1 minute 3000 x g).
- 7) With the exception of the substrate blank wells, do not allow wells to stand uncovered or dry for extended periods between incubation steps.

VI. ADDITIONAL BUFFERS & SOLUTIONS REQUIRED

Coating buffer: 0.1 M Carbonate/bicarbonate buffer pH 9.6

Solution A: 1.24 g $\text{Na}_2\text{CO}_3 \cdot \text{H}_2\text{O}$ in 100 ml distilled water

Solution B: 1.68 g NaHCO_3 in 200 ml distilled water

Take 70 ml of solution A, and add solution B until the pH is 9.6 (approximately 175 ml of solution B required)

The prepared buffer can be stored up to one week at 2-8°C.

PBS stock solution [20 x]: 0.2 M Phosphate Buffered Saline (PBS)

Dissolve	32 g	$\text{Na}_2\text{HPO}_4 \cdot 2\text{H}_2\text{O}$
	6 g	$\text{NaH}_2\text{PO}_4 \cdot 2\text{H}_2\text{O}$
	164 g	NaCl

in 900 ml distilled water (intensive stirring and some heating will speed dissolution).

Bring the temperature of the solution back to room temperature (18-25°C) and check pH; if necessary adjust pH to 6.8 - 6.9 with concentrated HCl or NaOH, and add distilled water to a volume of 1 liter (when diluted 20 times the obtained buffer will have a pH of 7.2 - 7.4).

Add 20 mg thiomersal as preservative. Do not use sodium azide (NaN_3) since this preservative reduces the quality of the enzymatic label.

The prepared buffer can be stored up to three months at 2-8°C.

Note: in the concentrated buffer salt crystals may appear when stored at 2-8°C. Before preparing the working-strength buffer, first warm the concentrated buffer BRIEFLY to 37°C to dissolve the precipitate.

Washing buffer: PBS with 0.005 % TWEEN 20

Make 1 liter of working-strength PBS by diluting the PBS stock solution (see above) 20-fold with distilled water.

Add 50 μl TWEEN 20.

The prepared buffer can be stored up to one month at 2-8°C.

Substrate buffer: 0.11 M acetate buffer pH 5.5

Dissolve 15.0 g sodium-acetate ($\text{CH}_3\text{COONa}\cdot 3\text{H}_2\text{O}$) in 800 ml distilled water.

Adjust pH to 5.5 with glacial acetic acid, add distilled water to a volume of 1 liter.

Do not add any preservative (e.g. merthiolate, sodium azide) since this may affect the quality of the enzymatic colour development.

The prepared buffer can be stored up to two weeks at 2-8°C.

3,5,3',5'-tetramethylbenzidine (TMB) stock solution: 6 mg/ml TMB in DMSO

Dissolve 30 mg 3,5,3',5'-tetramethylbenzidine (TMB) in 5 ml dimethylsulfoxide (DMSO).

The prepared stock solution can be stored up to 1 month **at room temperature (18-25°C)** and **protected against light**.

Hydrogen peroxide stock solution: 3% H_2O_2 solution in distilled water.

The prepared stock solution can be stored up to one month at 2-8°C.

Substrate solution

For each plate mix the following reagents:

12 ml substrate buffer

200 μl TMB stock solution

12 μl H_2O_2 stock solution

The substrate solution should be prepared just before use and has to be at room temperature (18-25°C) for optimal reproducible results.

Stop solution: 1.8 M H_2SO_4 solution in distilled water.

VII. ADDITIONAL INFORMATION

Additional materials required

- Pipetting devices for accurate delivery of 1-10 ml, 50 ml, 100 ml and 1 ml volumes.
- Beakers, flasks, cylinders necessary for preparation of reagents.
- Device for delivery of washing buffer (wash bottle / automated plate washer).
- Microtiter plate reader.

Sensitivity

MEAN calculated zero signal + 3 SD : 0.5 – 1.5 pg/ml (shake - static incubation)
2 x (MEAN calculated zero signal) : 1 – 3 pg/ml (shake - static incubation)

Note: the sensitivity is dependent upon the type and quality of enzymatic substrate.

Expected values

IL-13 values in fresh serum and plasma samples of healthy individuals are below 10 pg/ml.

Specificity

No crossreactivity was observed with the following recombinant human proteins: IL-1 α , IL-1 β , IL-2, IL-3, IL-4, IL-5, IL-6, IL-7, IL-8, IL-9, IL-10, IL-11, Macrophage Colony Stimulating Factor (M-CSF), Granulocyte Colony Stimulating Factor (G-CSF), Granulocyte/Macrophage Colony Stimulating Factor (GM-CSF), Leukaemia Inhibitory Factor (LIF), RANTES, Stem Cell Factor/ Mast Cell Factor (SCF/MCF), Transforming Growth Factor β -1 (TGF β -1), Tumour Necrosis Factor α , Tumour Necrosis Factor β (TNF β /Lymphotoxin), and Interferon γ (IFN γ).

REFERENCES

1. Mosmann, T.R. and Coffman, R.L. (1989) *Annu.Rev.Immunol.* 7: 145
2. Minty, A. *et al* (1993) *Nature* 362: 248
3. McKenzie, A.N.J. *et al* (1993) *Proc.Natl.Acad.Sci. USA* 90: 3735
4. Zurawski, G. and De Vries, J.E. (1994) *Immunol.Today* 15: 19
5. Zurawski, G. and De Vries, J.E. (1994) *Stem Cells* 12: 169
6. De Waal Malefyt, R. *et al* (1993) *J.Immunol.* 151: 6370
7. Defrance, T. *et al* (1994) *J.Exp.Med.* 179: 135
8. Punnonen, J. *et al* (1993) *Proc.Natl.Acad.Sci. USA* 90: 3730
9. Zurawski, G. *et al* (1993) *EMBO J.* 12: 2663
10. Jinquan, T.B. *et al* (1995) *J.Immunol.* 154: 3742
11. Van der Pouw Kraan, C.T.M. *et al* (1995) submitted
12. Labit-Le Bouteiller, C. *et al* (1995) *J.Immunol.Meth.* 181: 29
13. Thomson, A.W. (1991) *The cytokine handbook.* Academic Press ISBN 0-12-689660-7

VIII. ASSAY PROCEDURE

1. **BRING ALL REAGENTS TO ROOM TEMPERATURE (18-25°C)**, with the exception of the streptavidin-HRP conjugate which has to be kept at -18°C to -32°C to ensure stability. Centrifuge all vials before use (1 minute 3000 x g).

For your convenience an easy-reference manual with check list and plate plan are available on the last pages of this leaflet.

2. DILUTION BUFFER

The kit contains one bottle with 5-fold concentrated dilution buffer.

Calculate the quantity of dilution buffer required (approximately 15 ml undiluted buffer per microtiter plate) and prepare a working-strength solution by diluting the opalescent concentrated buffer 5 times in distilled water before use. The working-strength dilution buffer can be stored for up to one week at 2-8°C.

For optimal assay results, dilute samples and standard in working-strength dilution buffer.

3. MICROTITER PLATES

Coating antibody

Coating

The kit contains three microtiter plates for 96 tests each, including the standard curve samples.

Prepare coating buffer as described on page 3 of the information leaflet.

Per microtiter plate, add 120 µl of coating antibody (red-capped vial) to 12 ml coating buffer.

Add 100 µl to all wells, cover microtiter plate(s) with lid and **incubate overnight at room temperature (18-25°C)**.

Washing procedure

Prepare working-strength PBS (1:20 dilution of stock PBS as described on page 3 of the information leaflet).

Aspirate supernatants from wells and completely fill the wells (> 300 µl) with working-strength PBS and aspirate. Repeat this four times, after the final aspiration the wells should be dry.

Blocking procedure

The kit contains one transparent-capped vial with 2 ml blocking reagent.

Prepare blocking buffer by adding 500 µl blocking reagent to 25 ml working-strength PBS (1:20 dilution of stock PBS as described on page 3 of the information leaflet).

Add 200 µl blocking buffer to all wells, cover microtiter plate(s) with adhesive seal, gently agitate the microtiter plate by tapping the edge of the plate for a few seconds to mix contents of each well and **incubate for 1 hour at room temperature (18-25°C)**.

4. IL-13 STANDARD

Standard curve preparation

A natural human IL-13 standard has been calibrated against the WHO International Standard (IL-13 94/622; National Institute for Biological Standards and Control, Potters Bar, Hertfordshire, U.K. 1 WHO Unit = 1 ng IL-13).

The kit contains one lyophilized vial with 1000 pg/ml natural IL-13.

Reconstitute the lyophilized standard by adding 500 μ l of distilled water to the vial.

Incubate for 10 minutes at room temperature and mix gently. After reconstitution the standard must be kept cold (2-8°C) and stored frozen after use (<-18°C, preferably <-70°C).

Label 7 tubes, one tube for each dilutions: 125, 50, 20, 8, 3.2, 1.3 and 0.5 pg/ml.

Pipette 420 μ l of working-strength dilution buffer into the tube labelled 125 pg/ml and 300 μ l of workingstrength dilution buffer into the other tubes.

Transfer 60 μ l of the IL-13 standard (1000 pg/ml) into the first tube labelled 125 pg/ml, mix well and transfer 200 μ l of this dilution into the second tube labelled 50 pg/ml.

Repeat the serial dilutions five more times by adding 200 μ l of the previous tube of diluted standard to the 300 μ l of dilution buffer.

The standard curve will contain 125, 50, 20, 8, 3.2, 1.3, 0.5 and 0 pg/ml (dilution buffer).

It is recommended to prepare two separate series for each assay.

Avoid repeated freeze-thawing of the standard, although experimental data have shown that up to 3 freeze-thaw cycles have no effect on the huIL-13 levels of the standard.

5. SAMPLES

Serum, heparin or EDTA-anti-coagulated plasmas, and culture fluids are suitable for use in the assay. Do not use grossly haemolyzed or lipemic specimens. If samples are to be run within 24 hours, they may be stored at 2-8°C; otherwise samples should be stored frozen (<-18°C).

Up to 3 freeze-thaw cycles have no effect on the IL-13 levels of serum or plasma samples. Nonetheless, excessive freeze-thaw cycles should be avoided. Prior to the assay, frozen samples should be thawed **as quickly as possible** in a 37°C waterbath and then brought to room temperature (18-25°C).

It is recommended to dilute the test samples at least 1:2 in working-strength dilution buffer. If high levels of IL-13 (>200 pg/ml) are expected in the test samples, additional dilutions of sample i.e. 1:20 and 1:100 should also be prepared.

6. FIRST WASH STEP

Prepare washing buffer as described on page 3 of this leaflet.

Wash the required microtiter plates five times with washing buffer in a plate washer. In case of manual washing, completely fill the wells ($> 300 \mu\text{l}$) with washing buffer and aspirate, repeat this four times. After the final aspiration the wells should be dry.

7. FIRST INCUBATION STEP

Standards and samples

Leaving the substrate blank wells empty, transfer $100 \mu\text{l}$ of the prepared standards and samples in duplicate into the appropriate wells (see recommended plate plan).

Cover plate(s) with adhesive seal, gently agitate the microtiter plate by tapping the edge of the plate for a few seconds to mix contents of each well and **incubate for 1 hour at room temperature (18-25°C)**.

8. SECOND WASH STEP

Aspirate supernatant from wells and wash the microtiter plate(s) as described in point 6 above.

9. SECOND INCUBATION STEP

biotinylated antibody

The kit contains one yellow-capped vial with concentrated antibody-biotin conjugate.

Per microtiter plate, add $120 \mu\text{l}$ biotinylated antibody to 12 ml working-strength dilution buffer just before use.

Leaving the substrate blank wells empty, add $100 \mu\text{l}$ of diluted biotinylated antibody to all wells.

Cover plate(s) with adhesive seal, gently agitate the microtiter plate by tapping the edge of the plate for a few seconds to mix contents of each well and **incubate for 1 hour at room temperature (18-25°C)**.

10. THIRD WASH STEP

Aspirate supernatant from wells and wash the microtiter plate(s) as described in point 6 above.

11. THIRD INCUBATION STEP

Streptavidin-HRP conjugate

The kit contains one brown capped vial of concentrated streptavidin-HRP conjugate, which must be stored at -18°C to -32°C to maintain maximal stability. The contents of the vial will not be frozen at this temperature.

Per microtiter plate, add $3\ \mu\text{l}$ streptavidin-HRP conjugate to 30 ml of working-strength dilution buffer just before use. **Do not prepare in advance of assay.**

Leaving the substrate blank wells empty, add $100\ \mu\text{l}$ of streptavidin-HRP conjugate to all wells.

Cover the microtiter plate(s) with adhesive seal, agitate the microtiter plate by tapping the edge of the frame for a few seconds to mix contents of each well and **incubate for 30 minutes at room temperature ($18-25^{\circ}\text{C}$).**

12. FOURTH WASH STEP

Aspirate supernatant from wells and wash the microtiter plate(s) as described in point 6 above.

13. FOURTH INCUBATION STEP

Enzymatic colour development

Approximately 10 minutes before use, prepare the substrate solution as described on page 4 of this leaflet.

The substrate solution should be at room temperature ($18-25^{\circ}\text{C}$) for optimal reproducible results.

Add $100\ \mu\text{l}$ of substrate solution to all wells, **including the substrate blank wells.**

Cover microtiter plate(s) with lid, gently agitate the microtiter plate by tapping the edge of the frame for a few seconds to mix contents of each well and **incubate for 30 minutes at room temperature ($18-25^{\circ}\text{C}$) in the dark.**

do not cover the plate with aluminium foil.

Note: The speed of enzymatic colour development is influenced by many factors including temperature and quality of the used TMB.

14. STOP ENZYMATIC REACTION

Add 100 μ l of stop solution to all wells.

After stopping the colour is stable for maximally 30 minutes.

15. PLATE READ-OUT

Read at 450 nm in an ELISA reader.

IX. RESULTS

Substrate blank

- Record the absorbance at 450 nm for the substrate blank wells and average the duplicate values.

Standard curve


- Record the absorbance at 450 nm for each well containing standard and average the duplicate values.
- Calculate the net average absorbances by subtracting the average of the substrate blank wells.
- Plot the net average absorbances (ordinate) versus the IL-13 concentration in pg/ml (abscissa) on log-linear paper and draw the best fitting curve. An example of a standard curve is given on the next page.

Samples

- Record the absorbance at 450 nm for each standard well, and average the duplicate values.
- Calculate the net average absorbances by subtracting the average of the substrate blank wells.
- Locate the net average absorbance value found for each sample on the vertical axis and follow a horizontal line intersecting the standard curve. At the point of intersection, read the IL-13 concentration (pg/ml) from the horizontal axis. Multiply the obtained IL-13 concentration with the dilution factor of the sample and record this figure.

X. INCREASED SENSITIVITY

The assay sensitivity can be increased by a small adaptation of the incubation methodology. Just follow all the instructions as stated in the assay procedure (chapter VIII), but incubate at room temperature (18-25°C) on a horizontal plate shaker at 700 ± 100 rpm. All incubations, including the enzymatic colour development, have to be completed on the shaker, in the same time as stated in the static assay procedure. This will result in an increase in assay sensitivity, with small effects on the background levels (see figure next page).

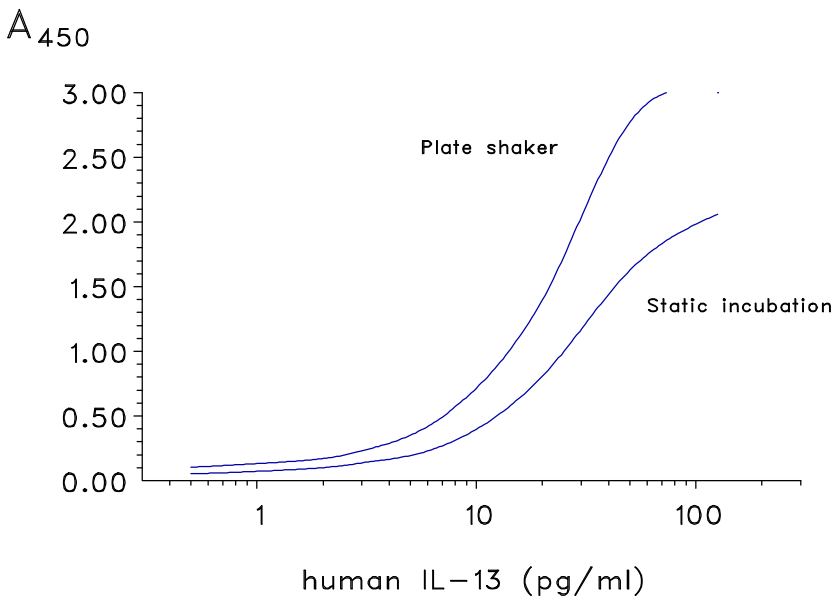

Typical standard curve for the PeliKine compact™ human IL-13 ELISA kit
 The assay is completed static or shaken at room temperature

	STATIC INCUBATION	SHAKEN INCUBATION
	Calculated mean absorbance at 450 nm	
substrate blank	0	0
0 pg/ml	0.036	0.065
0.5 pg/ml	0.053	0.104
1.3 pg/ml	0.081	0.144
3.2 pg/ml	0.158	0.289
8 pg/ml	0.314	0.573
20 pg/ml	0.808	1.394
50 pg/ml	1.627	2.772
125 pg/ml	2.030	≥ 3.000

DO NOT USE THESE DATA TO CONSTRUCT A STANDARD CURVE FOR SAMPLE VALUE CALCULATIONS

	1	2	3	4	5	6	7	8	9	10	11	12
A	S1	S1										
B	S2	S2										
C	S3	S3										
D	S4	S4										
E	S5	S5										
F	S6	S6										
G	S7	S7										
H	S8	S8									B	B

Plate plan proposed for the Pelikine compact™ human IL-13 ELISA kit:

Key: B: substrate blank S1-S8: IL-13 standards 0 - 125 pg/ml Empty: samples

Protocol summary and checklist PeliKine compactä human IL-13 ELISA kit

Day 0:

- Bring coating antibody to room temperature (18-25°C).
- Prepare coating buffer.
- Dilute coating antibody 1:100 in coating buffer, add 100 µl to all wells, cover the plate(s) and incubate overnight at room temperature.

Day 1:

- Bring all reagents, with the exception of streptavidin-HRP, to room temperature.
- Prepare blocking buffer
- Wash the plate(s) five times with PBS.
- Add 200 µl blocking buffer to all wells and incubate for one hour at room temperature.
- Prepare dilution buffer, standard and sample dilutions.
- Prepare washing buffer.
- Wash the plate(s) five times with washing buffer.
- Leaving the substrate blank wells empty, add 100 µl of standard and sample dilutions to the appropriate wells, cover the plate(s) and incubate for one hour at room temperature.
- Dilute biotinylated antibody 1:100 in dilution buffer.
- Wash the plate(s) five times with washing buffer.
- Leaving the substrate blank wells empty, add 100 µl of the diluted biotinylated antibody to all wells, cover the plate(s) and incubate for one hour at room temperature.
- Dilute the streptavidin-HRP conjugate 1:10,000 in dilution buffer.
- Wash the plate(s) five times with washing buffer.
- Leaving the substrate blank wells empty, add 100 µl of the streptavidin-HRP conjugate to all wells, cover plate(s) and incubate for 30 minutes at room temperature.
- Just before use, prepare substrate solution.
- Wash the plate(s) five times with washing buffer.
- Add 100 µl substrate solution to all wells, including the substrate blank wells, and incubate for 30 minutes at room temperature in the dark.
- Add 100 µl stop solution to all wells and read the plate at 450 nm.
- Calculate the amount of IL-13 in the samples.